

SUPERVISOR TEST




ORANGETOWN TOWN  
POLICE DEPT.  
DATAMASTER dmt: 115206

Date: 03/26/2020

OPERATOR NAME:  
JOSEPH W SULLIVAN  
Permit #: 46948  
Operator Agency/Dept: ORANGETOWN TOWN P.D.  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:25
INTERNAL STANDARD	VERIFIED	00:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:27
BLANK TEST	0.00	00:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:28
BLANK TEST	0.00	00:29

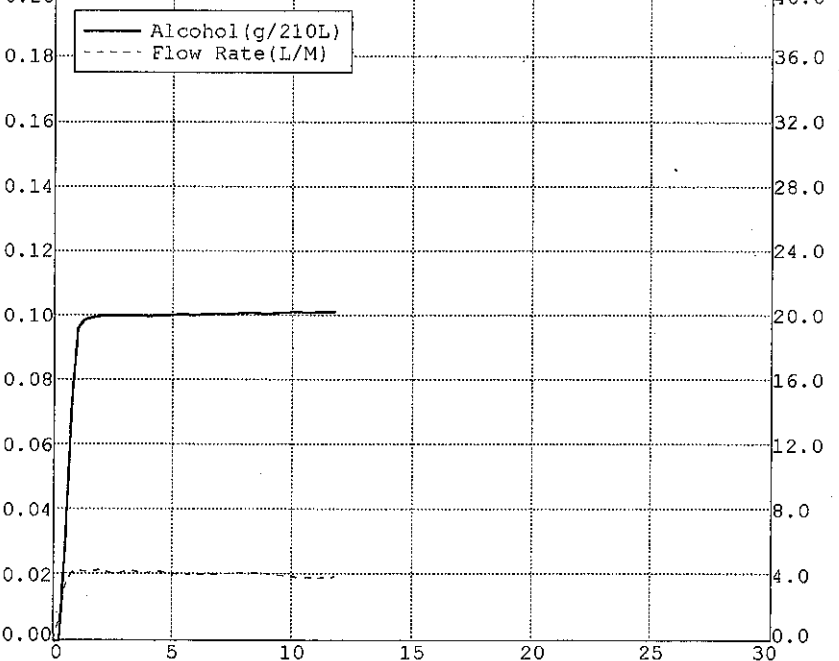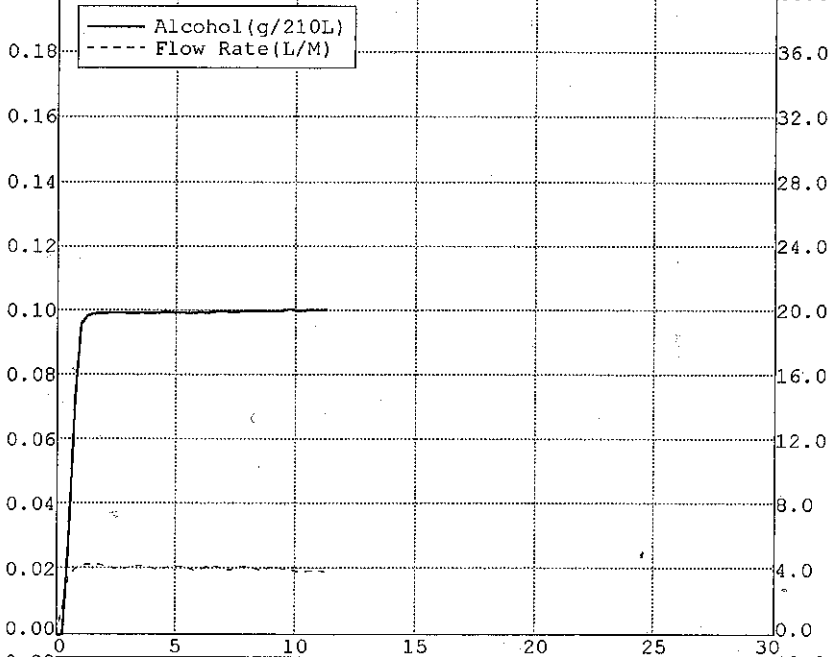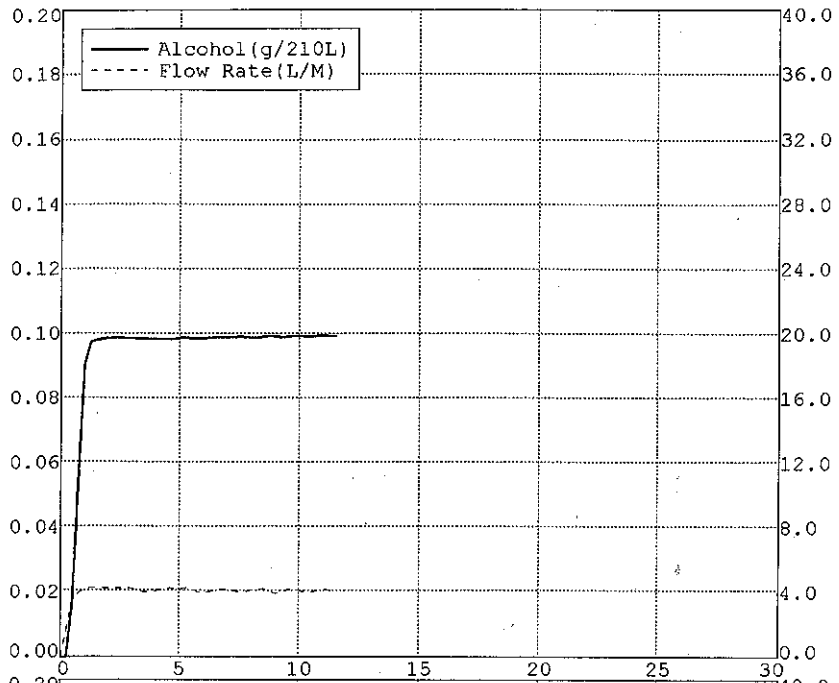

SUPERVISOR TEST

ORANGETOWN TOWN  
POLICE DEPT.  
DATAMASTER dmt: 115206

Date: 03/26/2020

OPERATOR NAME:  
JOSEPH W SULLIVAN  
Permit #: 46948  
Operator Agency/Dept: ORANGETOWN TOWN P.D.  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:25
INTERNAL STANDARD	VERIFIED	00:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:27
BLANK TEST	0.00	00:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:28
BLANK TEST	0.00	00:29

